


Tapered Implant Surgical Kits & Components Assembly

QNTSK Premium Kit




The Tapered Implant Surgical Tray

Simplicity In Site Preparation

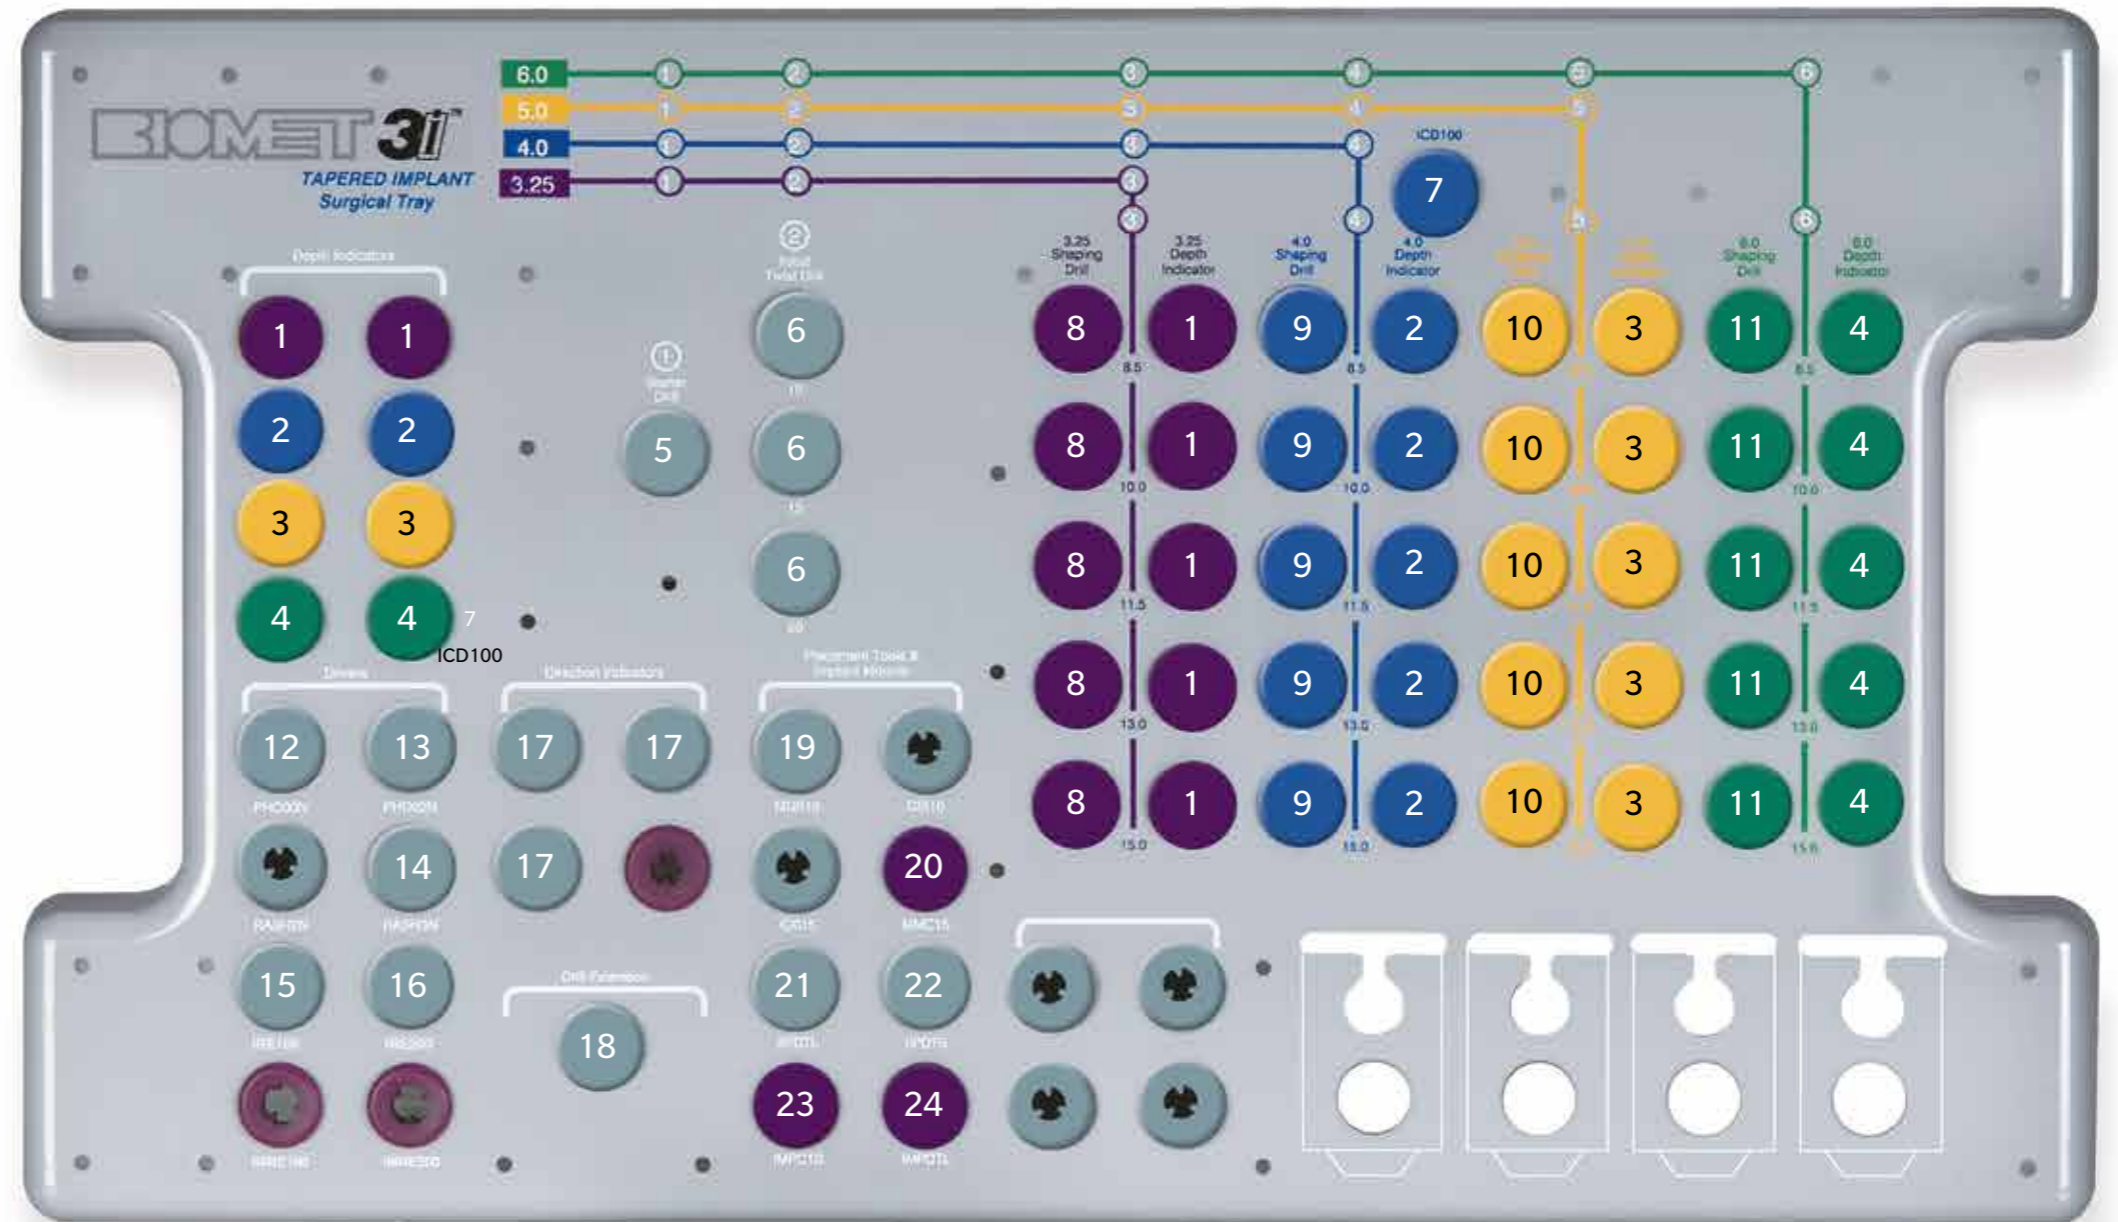

NOTE: Graphic Illustrates Component Location For QNTSK40 Premium Kit

Tapered Implant Dense Bone Tap Kit

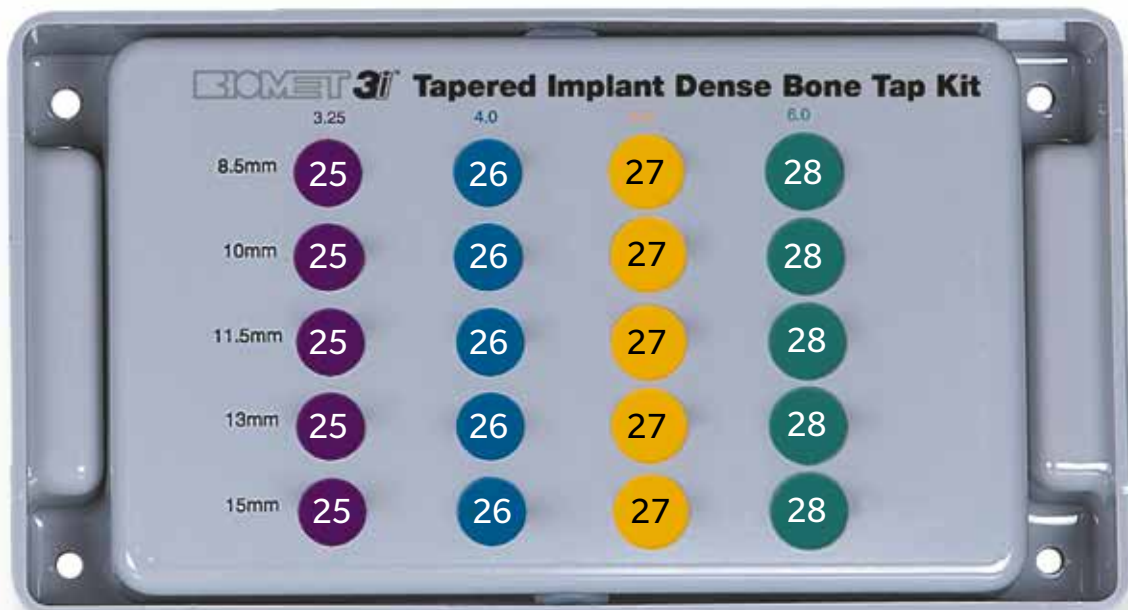

25

NTAP32XX



26

NTAP4XX



27

NTAP5XX



28

NTAP6XX

NOTE: Tapping in dense bone is required. Exceeding an insertion torque of more than 90 Ncm may deform or strip the driver tip or the implant's internal hex and may possibly delay the surgical procedure. Please refer to the Surgical Manual.

QNTSK Surgical Tray Contents

QNTSK40 Premium Kit			
QNTSK40U Upgrade Kit			
QNTSK20 Starter Kit			
	Description	Item #	
1	Tapered Implant Depth Indicator 3.25 mm(D) X 8.5 mm(L) 3 Ea.	NTDI3285	• • •
1	Tapered Implant Depth Indicator 3.25 mm(D) X 10 mm(L)	NTDI3210	• • •
1	Tapered Implant Depth Indicator 3.25 mm(D) X 11.5 mm(L)	NTDI3211	• • •
1	Tapered Implant Depth Indicator 3.25 mm(D) X 13 mm(L)	NTDI3213	• • •
1	Tapered Implant Depth Indicator 3.25 mm(D) X 15 mm(L)	NTDI3215	• • •
2	Tapered Implant Depth Indicator 4 mm(D) X 8.5 mm(L) 3 Ea.	NTDI485	• • •
2	Tapered Implant Depth Indicator 4 mm(D) X 10 mm(L)	NTDI410	• • •
2	Tapered Implant Depth Indicator 4 mm(D) X 11.5 mm(L)	NTDI411	• • •
2	Tapered Implant Depth Indicator 4 mm(D) X 13 mm(L)	NTDI413	• • •
2	Tapered Implant Depth Indicator 4 mm(D) X 15 mm(L)	NTDI415	• • •
3	Tapered Implant Depth Indicator 5 mm(D) X 8.5 mm(L) 3 Ea.	NTDI585	• • •
3	Tapered Implant Depth Indicator 5 mm(D) X 10 mm(L)	NTDI510	• • •
3	Tapered Implant Depth Indicator 5 mm(D) X 11.5 mm(L)	NTDI511	• • •
3	Tapered Implant Depth Indicator 5 mm(D) X 13 mm(L)	NTDI513	• • •
3	Tapered Implant Depth Indicator 5 mm(D) X 15 mm(L)	NTDI515	• • •
4	Tapered Implant Depth Indicator 6 mm(D) X 8.5 mm(L) 3 Ea.	NTDI685	• • •
4	Tapered Implant Depth Indicator 6 mm(D) X 10 mm(L)	NTDI610	• • •
4	Tapered Implant Depth Indicator 6 mm(D) X 11.5 mm(L)	NTDI611	• • •
4	Tapered Implant Depth Indicator 6 mm(D) X 13 mm(L)	NTDI613	• • •
4	Tapered Implant Depth Indicator 6 mm(D) X 15 mm(L)	NTDI615	• • •
5	ACT® Pointed Starter Drill	ACTPSD	• • •
6	ACT Reusable Twist Drill 2 mm(D) X 10 mm(L)	ACT2010	• • •
6	ACT Reusable Twist Drill 2 mm(D) X 15 mm(L)	ACT2015	• • •
6	ACT Reusable Twist Drill 2 mm(D) X 20 mm(L)	ACT2020	• • •
7	Certain® Countersink Drill, 4 mm(D)	ICD100	• • •
8	Quad Shaping Drill 3.25 mm(D) X 8.5 mm(L)	QSD3285	• • •
8	Quad Shaping Drill 3.25 mm(D) X 10 mm(L)	QSD3210	• • •
8	Quad Shaping Drill 3.25 mm(D) X 11.5 mm(L)	QSD3211	• • •
8	Quad Shaping Drill 3.25 mm(D) X 13 mm(L)	QSD3213	• • •
8	Quad Shaping Drill 3.25 mm(D) X 15 mm(L)	QSD3215	• • •
9	Quad Shaping Drill 4 mm(D) X 8.5 mm(L)	QSD485	• • •
9	Quad Shaping Drill 4 mm(D) X 10 mm(L)	QSD410	• • •
9	Quad Shaping Drill 4 mm(D) X 11.5 mm(L)	QSD411	• • •
9	Quad Shaping Drill 4 mm(D) X 13 mm(L)	QSD413	• • •
9	Quad Shaping Drill 4 mm(D) X 15 mm(L)	QSD415	• • •
10	Quad Shaping Drill 5 mm(D) X 8.5 mm(L)	QSD585	• • •
10	Quad Shaping Drill 5 mm(D) X 10 mm(L)	QSD510	• • •
10	Quad Shaping Drill 5 mm(D) X 11.5 mm(L)	QSD511	• • •
10	Quad Shaping Drill 5 mm(D) X 13 mm(L)	QSD513	• • •
10	Quad Shaping Drill 5 mm(D) X 15 mm(L)	QSD515	• • •
11	Quad Shaping Drill 6 mm(D) X 8.5 mm(L)	QSD685	• • •
11	Quad Shaping Drill 6 mm(D) X 10 mm(L)	QSD610	• • •
11	Quad Shaping Drill 6 mm(D) X 11.5 mm(L)	QSD611	• • •

QNTSK40 Premium Kit			
QNTSK40U Upgrade Kit			
QNTSK20 Starter Kit			
	Description	Item #	
11	Quad Shaping Drill 6 mm(D) X 13 mm(L)	QSD613	• • •
11	Quad Shaping Drill 6 mm(D) X 15 mm(L)	QSD615	• • •
12	Narrow Posterior Hexed Driver - 17 mm(L)	PHD00N	• • •
13	Posterior Large Hexed Driver - 17 mm(L)	PHD02N	• • •
14	Narrow Right Angle Large Hexed Driver Tip - 24 mm(L)	RASH3N	• • •
15	Certain Universal Ratchet Ext. Driver 4.1, 5, 6 mm(D) - Short	IRE100U	• • •
16	Certain Universal Ratchet Ext. Driver 4.1, 5, 6 mm(D) - Long	IRE200U	• • •
17	Direction Indicator 2 mm(D) X 10 mm(L) 3 Ea.	DI100	• • •
18	ACT Drill Extension	ACTDE	• • •
19	Handpiece Connector	MDR10	• • •
20	Implant Mount 3.4 mm(D) X 15 mm(L)	MMC15	• • •
21	Certain Implant Driver Tip 4, 5, 6 mm(D) - Long	IIPDTL	• • •
22	Certain Implant Driver Tip 4, 5, 6 mm(D) - Short	IIPDTS	• • •
23	Certain Implant Driver Tip 3.4 mm(D) - Short	IMPDTL	• • •
24	Certain Implant Driver Tip 3.4 mm(D) - Long	IMPDTL	• • •
25	Tapered Implant Dense Bone Tap 3.25 mm(D) X 8.5 mm(L)	NTAP3285	• • •
25	Tapered Implant Dense Bone Tap 3.25 mm(D) X 10 mm(L)	NTAP3210	• • •
25	Tapered Implant Dense Bone Tap 3.25 mm(D) X 11.5 mm(L)	NTAP3211	• • •
25	Tapered Implant Dense Bone Tap 3.25 mm(D) X 13 mm(L)	NTAP3213	• • •
25	Tapered Implant Dense Bone Tap 3.25 mm(D) X 15 mm(L)	NTAP3215	• • •
26	Tapered Implant Dense Bone Tap 4 mm(D) X 8.5 mm(L)	NTAP485	• • •
26	Tapered Implant Dense Bone Tap 4 mm(D) X 10 mm(L)	NTAP410	• • •
26	Tapered Implant Dense Bone Tap 4 mm(D) X 11.5 mm(L)	NTAP411	• • •
26	Tapered Implant Dense Bone Tap 4 mm(D) X 13 mm(L)	NTAP413	• • •
26	Tapered Implant Dense Bone Tap 4 mm(D) X 15 mm(L)	NTAP415	• • •
27	Tapered Implant Dense Bone Tap 5 mm(D) X 8.5 mm(L)	NTAP585	• • •
27	Tapered Implant Dense Bone Tap 5 mm(D) X 10 mm(L)	NTAP510	• • •
27	Tapered Implant Dense Bone Tap 5 mm(D) X 11.5 mm(L)	NTAP511	• • •
27	Tapered Implant Dense Bone Tap 5 mm(D) X 13 mm(L)	NTAP513	• • •
27	Tapered Implant Dense Bone Tap 5 mm(D) X 15 mm(L)	NTAP515	• • •
28	Tapered Implant Dense Bone Tap 6 mm(D) X 8.5 mm(L)	NTAP685	• • •
28	Tapered Implant Dense Bone Tap 6 mm(D) X 10 mm(L)	NTAP610	• • •
28	Tapered Implant Dense Bone Tap 6 mm(D) X 11.5 mm(L)	NTAP611	• • •
28	Tapered Implant Dense Bone Tap 6 mm(D) X 13 mm(L)	NTAP613	• • •
28	Tapered Implant Dense Bone Tap 6 mm(D) X 15 mm(L)	NTAP615	• • •
	Open End Wrench*	CW100	• • •
	Certain Driver Replacement O-Rings (10-Pack)*	IRORDR	• • •
	Tapered Implant Dense Bone Tap Kit Tray*	NTAPKT	• • •
	Ratchet Extension Short 6 mm(L)*	RE100	• • •
	Ratchet Extension Long 15 mm(L)*	RE200	• • •
	Ratchet Wrench*	WR150	• • •
	Base, Molded Insert & Smoked Lid*	QNTSKT	• • •
	Implant Depth Gauge 20 mm(L)*	DPO20	• • •

* Items not pictured in this brochure.



Contact us at 1-800-342-5454 or visit

zimmerbiometdental.com

Zimmer Biomet Dental
Global Headquarters
4555 Riverside Drive
Palm Beach Gardens, FL 33410
Tel: +1-561-776-6700
Fax: +1-561-776-1272

Unless otherwise indicated, as referenced herein, all trademarks are the property of Zimmer Biomet; and all products are manufactured by one or more of the dental subsidiaries of Zimmer Biomet Holdings, Inc., and distributed and marketed by Zimmer Biomet Dental (and, in the case of distribution and marketing, its authorized marketing partners). For additional product information, please refer to the individual product labeling or instructions for use. Product clearance and availability may be limited to certain countries/regions. This material is intended for clinicians only and does not comprise medical advice or recommendations. This material may not be copied or reprinted without the express written consent of Zimmer Biomet Dental. ZBINST1096 REV A 09/17 ©2017 Zimmer Biomet, All rights reserved.

